

## **Impact of Storage Conditions on the Efficacy of Malaria Rapid Diagnostic Tests in Tropical Settings**

### **Abstract**

Malaria remains a significant global health challenge, with Nigeria bearing the highest burden. This study evaluated the impact of storage conditions on the performance of commercially available malaria rapid diagnostic tests (RDTs) in Uyo Local Government Area, Akwa Ibom State, Nigeria. Malaria prevalence was assessed across five health stations using CareStart™ pLDH/HRP-2 and HRP-2 RDTs. Blood samples were collected from patients under informed consent, and RDTs were stored under low (14.5°C-23.5°C) and moderate (24.6°C-34.5°C) temperatures, and varying humidity levels. Sensitivity, specificity, positive predictive values (PPVs), and negative predictive values (NPVs) of RDTs were compared with microscopy, chi-square was used to compare the relationship between variables with significant value at  $p < 0.05$ .

Results showed that temperature significantly impacted HRP-2 RDTs at some stations, while pLDH/HRP-2 RDTs were less affected. Humidity had a significant negative effect on RDT performance, especially under high humidity conditions. Overall, HRP-2 and pLDH/HRP-2 RDTs showed varying sensitivity and specificity across different storage conditions, with some stations recording significantly lower performance. Sensitivity ranged from 44.0% to 85.0% for HRP-2 and 61.3% to 90.0% for pLDH/HRP-2 across the stations. 26/53, 85/172, and 128/165 of pLDH/HRP-2 were stored in low, medium, and high humidity. The overall mean between RDTs and humidity was statistically significant ( $p < 0.05$ ). 155/336 and 34/54, for HRP-2 stored at low and moderate temperatures. The overall mean between HRP-2 and temperature was statistically significant ( $\chi^2 = 5.277$ ,  $df=1$ ,  $p = 0.022$ ).

Exposure to high temperatures and humidity can degrade the test components, reducing their accuracy. The findings show the need for regular quality control and appropriate storage of RDTs to maintain their efficacy and support malaria control efforts in Nigeria and other affected regions.

**Keywords:** Humidity, Malaria, mRDTs, Temperature

### **Introduction**

A report from a globally recognized public health organization shows that there are 241 million estimated cases of malaria in the world, this global record spread across eighty-five endemic countries, of which Nigeria takes the largest share (Temiloluwa et al., 2023). This current data showed that there was an increase of 14 million cases of malaria in the world compared to the previously estimated value of 227 million cases. This sharp increase could have been attributed to the outbreak experienced with the global pandemic of COVID-19 in the world. Meanwhile, between 2000 and 2015, there was a reduction in the incidence of malaria in the world; however, the number of incidences also witnessed an increase between 2019 and 2020, and this increase has also been linked to the global shutdown that the world experience during the period of increase in the incidence of malaria cases (Venkatesan, 2024). A total of 562,000 people died of malaria in 2015 while the total death due to malaria was 558,000 individuals in 2019. Besides, the estimated death rate increased by 12% in the year 2020 to 627,000 individuals. This increase has also been attributed to the effect of the COVID-19 pandemic that ravaged the whole world during this period. The estimated number of people at risk of death per one hundred thousand populations dropped to 13 individuals in 2019 from 15 people per one hundred thousand risks in 2015. Currently, the number of an individual at risk of death per one hundred thousand has increased to 15 individuals.

Almost all countries with the highest malaria burden are in the African region. Nigeria accounts for the highest burden at 27%, followed by the Democratic Republic of the Congo at 12%, and Uganda at 5% (Brunner et al., 2022). Nigeria remains the epicenter of malaria infection in Africa. The infection is one of the major causes of morbidity and mortality in Nigeria, with many children and adults reporting for malaria diagnosis and treatment in tertiary, secondary, primary, and private health facilities in the country (Morakinyo et al., 2018). Severe malaria in children, adolescent,

and some cases among adults often present with extreme weakness, impaired consciousness in some cases, anaemia, respiratory distress, convulsions in many children, hypoglycemia, and other symptoms that are associated with severe cases of malaria infection (Morakinyo et al., 2018). World Health Organization recommended that the gold standard for malaria diagnosis is the use of microscopy; however, some factors are potentially affecting the use of microscopy in the diagnosis of malaria infection in endemic areas, such factors include: well trained and adequately expertise microscopists, labour-intensive (Oboh et al., 2021), well-maintained quality reagent, high-quality binocular microscopes, and above all, it's time consuming (Venkatesan, 2024).

Other laboratory methods for diagnosing malaria, including polymerase chain reaction (PCR) and enzyme-linked immunosorbent assay (ELISA), are costly and necessitate well-equipped lab facilities with highly trained personnel (Persing et al., 2016). In Nigeria, these diagnostic techniques are limited to hospitals with substantial financial resources. However, immunochromatographic rapid diagnostic tests (RDTs) offer a viable alternative for diagnostic services in settings where the financial power is low. Malaria rapid diagnostic test measures the level of parasite-derived proteins in the bloodstream, the method is often recommended when there is no reliable microscopy method/expertise, or when the number of health care seeking individuals is high (Ajakaye & Ibukunoluwa, 2020). RDT method is relatively less time-consuming compared to microscopy and it could be carried out by personnel with limited training (Oladosu et al., 2021; Uba et al., 2021). When RDTs were designed, their function is often parasite species-specific or genus-specific, by detecting the expressed antigens by the different species of the malaria parasite (Wongsrichanalai et al., 2007). The antigens detected by various malaria RDTs include *P. falciparum* histidine-rich protein 2 (*PfHRP2*), *P. falciparum*-specific lactate dehydrogenase

(LDH), *P. vivax*-specific LDH, pan-LDH, and pan-aldolase (Barber et al., 2013; Bouyou-Akotet et al., 2013).

RDTs are sensitive to environmental conditions, especially temperature and humidity (Martíáñez-Vendrell et al., 2022). Antibodies and antigens can get denatured when exposed to high temperatures, which reduces their specificity and sensitivity. Over time, test components may deteriorate as a result of high humidity (Chiodini et al., 2007). However, extended exposure to light, particularly in the form of intense sunshine, can cause the chemicals and materials employed in RDTs to degrade. This may lead to poorer test findings and, in rare instances, false-positive outcomes. Unlike flow-through tests (involve movement through the membrane), lateral flow test involves the movement of the samples along the nitrocellulose strip (Abu et al., 2023). As a result of this design, malaria RDTs are heat-stable, however, if the temperature exceeds certain threshold, they tend to underperform. Furthermore, their operation is also impaired by cold environment, as the gold conjugate gets damaged by temperature below 0°C. Meanwhile, these RDTs can stay for as long as more than 18 months and remain active in their operation. RDTs have an expiration date that often serves as a reminder of their shelf life. Because the components of expired RDTs may deteriorate with time, using them can result in lower specificity and sensitivity. Consequently, regular quality control procedures are crucial. Based on the aforementioned, this study was designed to understand the effect of storage condition likely to be encountered during operational use in endemic areas on the commercially available malaria RDTs in Uyo Local Government Area.

## **Material and Methods**

Akwa Ibom State is situated in the South-South geopolitical zone of Nigeria. It is bordered by Cross River State to the east, Abia State to the north, Rivers State to the west, and the Atlantic Ocean to the south. The state enjoys a tropical rainforest climate, characterized by high humidity and heavy rainfall. The state experiences two main seasons: the rainy season (March to November) and the dry season (December to February). The temperature is between 22.2<sup>0</sup>C and 40.1<sup>0</sup>C (Aigbodion & Uyi, 2013). According to the 2006 census, Akwa Ibom had a population of approximately 3.9 million people. Current estimates indicate that the population has grown significantly. The state is predominantly inhabited by the Ibibio, Annang, Oron, and Eket ethnic groups, each with its own language, culture, and traditions. The state is one of Nigeria's leading oil-producing states, contributing significantly to the nation's oil and gas output. The state has numerous oil fields and is home to several major oil companies. The state has a growing industrial sector, with industries ranging from food processing to petrochemicals.

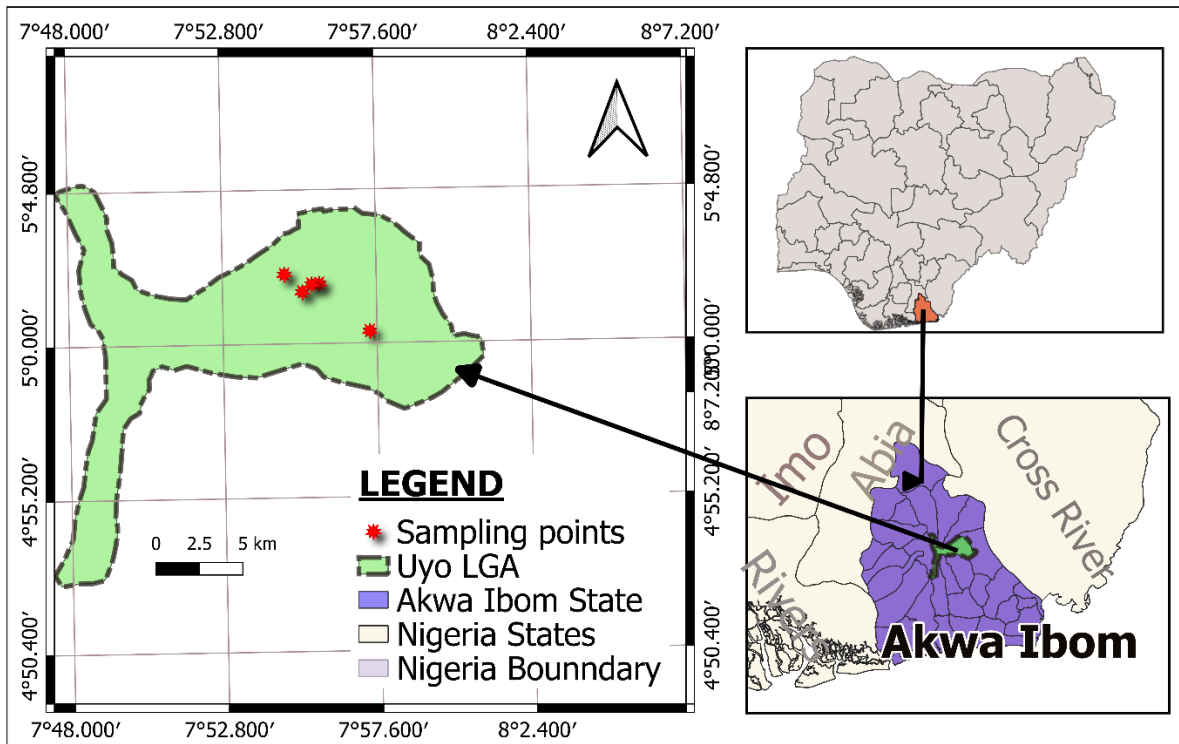


Fig. 1: Map of Uyo LGA

### Study Population

The study subjects were all patients who visited health centres with a request form for a malaria diagnosis at the relevant stations. Children under 10 years old who had parental or guardian permission and who came with them to the registration/sample collection location were taken into consideration.

### Blood sample collection and storage condition

All blood samples used were derived from a single patient who presented for a malaria infection test at each station. The samples were collected after obtaining informed consent and with the approval of the institutional ethical review committee. Two commercially available RDTs

(CareStart™ and SD Bionline) were studied: one designed to detect pLDH, while the other designed to detect pLDH/HRP-2. Upon delivery to the health stations, malaria RDTs were stored in accordance with the manufacturer's guidelines in non-air-conditioned environments, then allocated to separate groups for storage under the following temperatures: moderate (14.5°C-23.5°C) and high (24.6°C-34.5°C) for up to three weeks. The range of temperature used in this study were same as those found on various shelves where the RDTs are procured for normal laboratory procedures. Prior to the start of the study, the incubators were stabilized at the required temperature for three days before placing the RDTs to be tested inside. At scheduled time intervals, RDTs were taken out of storage and allowed to reach room temperature for 1 to 2 hours before testing. They were then used according to the manufacturer's instructions. To minimize inter-operator variability, the same personnel conducted the test readings at each station. Due to the different formats of the products, blinding the technicians to the results of other products was not feasible. However, each station was kept blinded to the results from other stations until the study was completed. Afterward, according to Williams *et al.* (2009), RDTs were subjected to one of the following conditions: air-dried for 2 hours and stored with the desiccant provided in their original packaging (low humidity); air-dried and stored without desiccant (moderate humidity); or stored without air-drying with wet tissue paper (high humidity). In addition, thick blood films were prepared, stained, and examined under the microscope by two experienced medical laboratory scientists.


## **Data analysis**

Data entry and cleaning were performed in spreadsheet, then exported to R for analysis. The dataset included participant demographics, parasite types, and RDT results. Sensitivity, specificity, positive predictive values (PPVs), and negative predictive values (NPVs) of the RDT compared to

microscopy were calculated with 95% confidence intervals (CI). According to WHO (2000) guidelines, RDTs must have at least 95% sensitivity and 90% specificity. Malaria prevalence was analyzed by stations. Data were presented in tables, graph, with statistical significance determined using the Pearson Chi-square test and a p-value threshold of 0.05.

**Results**

The ratios of total malaria positive cases were 134/390, 189/390, 239/390, and 278/390 by clinical, HRP-2, pLDH/HRP-2, and microscopy methods. The prevalence of malaria infection across all age groups of respondents was less than half by clinical method while the prevalence was more than half across all ages by pLDH/HRP-2 and microscopy methods (Figure 2).

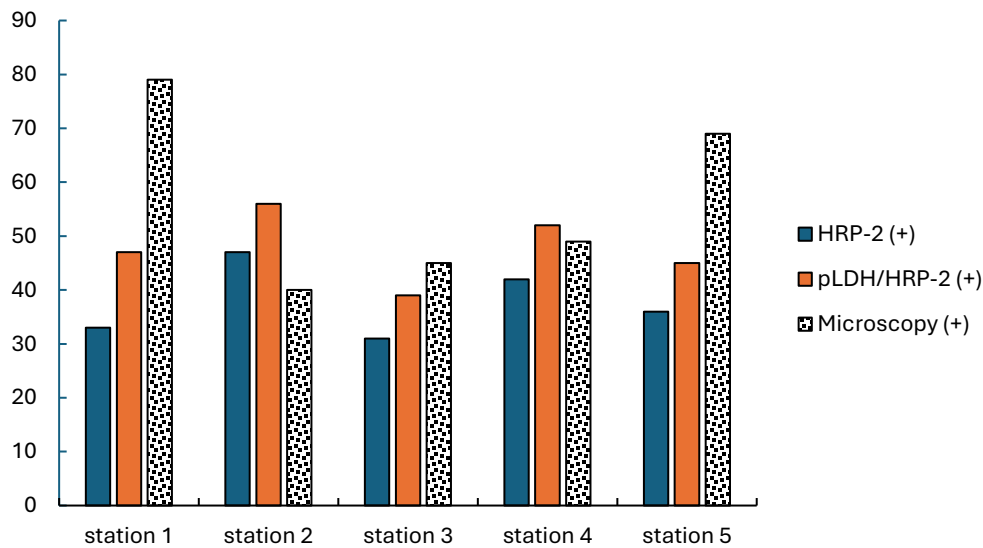

**Fig. 2: Prevalence of Malaria Parasites Infection based on sampling stations**

Temperature was categorized to low (14.5°C- 23.5°C) and moderate (24.6°C-34.5°C) during the study. In Station 1 hospital, all the RDTs (CareStart™ pLDH/HRP-2 and HRP-2) stored under



moderate temperature tested positive to malaria parasite while more than half off the CareStart™ pLDH/HRP-2 stored under low temperature tested positive to malaria infection. A significant difference occurred between temperature and HRP-2 RDT ( $\chi^2 = 7.441$ ,  $df=1$ ,  $p = 0.006$ ) (Table 2) but the difference between temperature and CareStart™ pLDH/HRP-2 was not significant ( $\chi^2 = 3.634$ ,  $df=1$ ,  $p = 0.057$ ). In station 2, A large proportion of the HRP-2 (43/74) and pLDH/HRP-2 (53/62) stored under low temperature tested positive to malaria parasites (Table 2). The observed differences in the means of pLDH/HRP-2 and temperature was statistically significant ( $\chi^2 = 4.740$ ,  $df=1$ ,  $p = 0.029$ ) but the mean difference between temperature and HRP-2 was not significant ( $p > 0.05$ ). A large percentage of both single and pLDH/HRP-2 RDTs stored under moderate temperature, tested positive to malaria parasites while the proportion of HRP-2 stored under low temperature was below average (42.4%). The mean difference of both single and combo RDTs in relation to storage temperature was not significant in station 3 (Table 2). A low proportion (20.0%) of CareStart™ pLDH/HRP-2 stored under moderate temperature tested positive to malaria parasites while no HRP-2 RDT stored under moderate temperature tested positive to malaria parasite in station 4 (Table 2). Meanwhile, more than half of both single and combo RDTs stored under low temperature tested positive to malaria parasites in station 4. On the other hand, more than half of HRP-2 and pLDH/HRP-2 RDTs stored under moderate temperature, tested positive to malaria parasites in station 5 (Table 2). In stations 4 and 5, the means difference for both HRP-2 and pLDH/HRP-2 RDTs in relation to temperature were statistically significant ( $p < 0.05$ ). The overall prevalence of malaria parasites by HRP-2 and pLDH/HRP-2 RDTs in relation to the storage temperature is represented in Table 2. A total proportion, 155/336 and 34/54, of HRP-2 stored under low and moderate temperature were reported in this study. The overall mean between

HRP-2 and temperature was statistically significant ( $\chi^2 = 5.277$ ,  $df=1$ ,  $p = 0.022$ ) but pLDH/HRP-2 RDTs and temperature did not show any significant difference.

**Table 2: Prevalence of Malaria Parasites Infection based on temperature**

	Station 1		Station 2		Station 3		Station 4		Station 5	
Temperature	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)
Low	28 (37.8)	42 (56.8)	43 (58.1)	53 (71.6)	28 (37.8)	36 (48.6)	42 (56.8)	51 (68.9)	32 (43.2)	40 (54.1)
Medium	5 (100)	5 (100)	4 (66.7)	3 (50.0)	3 (60.0)	3 (60.0)	0 (0.0)	1 (20.0)	4 (80.0)	5 (100)
Total	33 (41.8)	47 (59.5)	47 (69.1)	56 (82.4)	31 (43.7)	39 (54.9)	42 (53.2)	52 (65.8)	36 (38.7)	45 (48.4)
Chi-square	7.441	3.634	0.018	4.740	0.584	0.056	6.059	4.982	16.851	22.891
P-value	0.006	0.057	0.605	0.029	0.445	0.813	0.014	0.026	0.001	0.001

Humidity was divided into low, medium, and high during the study. In station 1, CareStart™ pLDH/HRP-2 RDT stored under low, medium, and high humidity tested positive to between 50% and 68.3% malaria cases while HRP-2 RDT tested positive to 41.8% of the overall malaria cases (Table 3). There was no significant difference between humidity and RDTs (HRP-2 and CareStart™ pLDH/HRP-2). In station 2, A large proportion of pLDH/HRP-2 stored under low (3/5), medium (28/34), and high (25/29) humidity tested positive to malaria parasites (Table 3). The observed differences in the means of RDTs (HRP-2 and pLDH/HRP-2) and humidity was not statistically significant ( $p > 0.05$ ). For HRP-2 stored under low, medium, and high humidity in station 3, less than half tested positive to malaria parasite under low and medium humidity; however, pLDH/HRP-2 stored under low and high humidity tested positive to a high proportion of malaria parasite. The mean difference of both single and combo RDTs in relation to humidity was not significant in station 3 (Table 3). A low proportion (38.2%) of CareStart™ pLDH/HRP-2 stored under medium humidity tested positive to malaria parasites while no HRP-2 RDT stored under same humidity tested positive to low (32.4%) proportion of malaria parasite in station 4

(Table 3). Meanwhile, more than half of CareStart™ pLDH/HRP-2 RDTs stored in high humidity tested positive to malaria parasites in station 5. In stations 4 and 5, the means difference for both HRP-2 and pLDH/HRP-2 RDTs in relation to humidity were statistically significant ( $p < 0.05$ ). The overall prevalence of malaria parasites by HRP-2 and pLDH/HRP-2 RDTs in relation to the humidity is shown in Table 3. A total proportion, 26/53, 85/172, and 128/165 of pLDH/HRP-2 stored in low, medium, and high humidity were recorded in this study. The overall mean between RDTs (HRP-2 and pLDH/HRP-2) and humidity was statistically significant ( $p < 0.05$ ).

**Table 3: Prevalence of Malaria Parasites Infection based on Humidity**

Humidity	No. Examined	Station 1		Station 2		Station 3		Station 4		Station 5	
		HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)	HRP-2 (%)	pLDH/HRP-2 (Combo) (%)
Low	8	3 (37.5)	4 (50.0)	2 (40.0)	3 (60.0)	3 (30.0)	6 (60.0)	5 (62.5)	7 (87.5)	6 (27.3)	6 (27.3)
Medium	30	8 (26.7)	15 (50.0)	25 (73.5)	28 (82.4)	15 (41.7)	17 (47.2)	11 (32.4)	13 (38.2)	8 (21.1)	12 (31.6)
High	41	22 (53.7)	28 (68.3)	20 (69.0)	25 (86.2)	13 (52.0)	16 (64.0)	26 (70.3)	32 (86.5)	22 (66.7)	27 (81.8)
Chi-square		5.256	2.738	2.117	1.689	1.524	1.798	10.776	20.196	17.078	22.994
P-value		0.072	0.254	0.347	0.430	0.467	0.407	0.005	0.001	0.001	0.001

On comparing the performance of HRP-2 test with the malaria diagnostic method, the sensitivity of HRP-2 for station 1, station 2, station 3, station 4, and station 5 were 44.0%, 85.0%, 51.1%, 69.4%, and 52.2 % respectively (Table 4). The specificity for station 1 hospital, station 2, station 3, station 4, and station 5 were 100%, 53.6%, 69.2%, 73.3%, and 100% respectively. The highest Positive Predictive Value (PPV) of 100% each was recorded for station 1 hospital and station 5; however, lowest Negative Predictive Value (NPV) of 8.7% was recorded for station 1. The highest Positive Likelihood Ratio (PLR) of 2.6 (95% CI: 1.4-4.85) was recorded in station 4 (Table 4).

**Table 4: Sensitivity, Specificity, Predictive values of HRP-2 Rapid Diagnostic Test using microscopy as the standard**

Health facility	Positive (%)	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	Positive Likelihood Ratio (95% CI)	Negative Likelihood Ratio (95% CI)	Accuracy (95% CI)
Station 1	33 (41.8)	44 (32.6-55.9)	100 (39.8-100)	100 (89.4-100)	8.7 (2.4-20.7)	-	0.56 (0.46-0.68)	46.8 (35.5-58.4)
Station 2	47 (69.1)	85 (70.2-94.3)	53.6 (33.9-72.5)	72.3 (57.4-84.4)	71.4 (47.8-88.7)	1.83 (1.2-2.8)	0.28 (0.1-0.6)	72.1 (59.9-82.3)
Station 3	31 (43.7)	51.1 (35.8-66.3)	69.2 (48.2-85.7)	74.2 (55.4-88.1)	45.0 (29.3-61.5)	1.7 (0.9-3.2)	0.71 (0.5-1.1)	57.6 (45.4-69.4)
Station 4	42 (53.2)	69.4 (54.6-81.8)	73.3 (54.1-87.7)	81.0 (65.9-91.4)	59.5 (42.1-75.3)	2.6 (1.4-4.85)	0.4 (0.3-0.7)	70.9 (59.6-80.6)
Station 5	36 (38.7)	52.2 (39.8)	100 (85.8-100)	100 (90.3-100)	42.1 (29.1-55.9)	-	0.5 (0.4-0.6)	64.5 (53.9-74.2)

The performance of pLDH/HRP-2 test when compared with the malaria diagnostic method, the sensitivity of pLDH/HRP-2 for station 1, station 2, station 3, station 4, and station were 61.3%, 90.0%, 66.7%, 77.6%, and 62.3 % respectively (Table 5). The highest specificity value of 91.7% was recorded for station 5 while the least value of 28.6% occurred in station 2. The highest Positive Predictive Value (PPV) of 97.9% was recorded for station 1; however, lowest Negative Predictive Value (NPV) of 45.8% was recorded for station 5. The highest Positive Likelihood Ratio (PLR) of 7.5 (95% CI: 2.0-28.6) was recorded in station 5. The highest pLDH/HRP-2 test accuracy of 69.9% was recorded for Station 5.

**Table 5: Sensitivity, Specificity, Predictive values of pLDH/HRP-2 Rapid Diagnostic Test using microscopy as the standard**

Health facility	Positive (%)	Sensitivity (95% CI)	Specificity (95% CI)	PPV (95% CI)	NPV (95% CI)	Positive Likelihood Ratio (95% CI)	Negative Likelihood Ratio (95% CI)	Accuracy (95% CI)
Station 1	47 (59.5)	61.3 (49.4-72.4)	75.0 (19.4-99.4)	97.9 (88.7-100)	9.4 (2.0-25.0)	2.5 (0.5-13.5)	0.5 (0.3-1.0)	62.0 (50.4-72.3)
Station 2	56 (82.4)	90.0 (76.3-97.2)	28.6 (13.2-48.7)	64.3 (50.4-76.6)	66.7 (34.6-90.1)	1.3 (1.0-1.6)	0.4 (0.1-1.1)	64.7 (52.2-75.9)
Station 3	39 (54.9)	66.7 (51.1-80.0)	65.4 (44.3-82.9)	76.9 (60.7-88.9)	53.1 (34.7-70.9)	1.9 (1.1-3.4)	0.5 (0.3-0.8)	66.2 (54.0-77.0)
Station 4	52 (65.8)	77.6 (63.4-88.2)	53.3 (34.3-71.7)	73.1 (59.0-84.4)	59.3 (38.8-77.6)	1.7 (1.1-2.5)	0.4 (0.2-0.8)	68.4 (56.9-78.4)
Station 5	45 (48.4)	62.3 (49.8-73.7)	91.7 (73.0-99.0)	95.6 (84.9-99.5)	45.8 (31.4-60.8)	7.5 (2.0-28.6)	0.4 (0.3-0.6)	69.9 (59.5-79.0)

## Discussion

As per the ASSURED criteria, the ideal rapid test should be: A = affordable, S = sensitive, S = specific, U = user-friendly (easy to perform with minimal steps and training), R = robust and rapid, E = equipment-free or requiring minimal equipment, and D = deliverable to those in need (Peeling & Mabey, 2010). We evaluated the temperature and humidity robustness of a malaria RDT brand and found that, despite the varying incubator temperatures, three stations showed no significant changes in test results, while two stations experienced a significant effect. Exposure to heat, humidity, or other adverse conditions can lead to decreased test accuracy (Martínez-Vendrell et al., 2022b). A study by Chiodini et al. (2007) demonstrated that tests based on *P. falciparum* histidine-rich protein-2 (HRP-2) maintained their sensitivity after exposure to high temperatures, whereas those based on *Plasmodium* lactate dehydrogenase (pLDH) exhibited reduced sensitivity under the same conditions.

Factors such as epidemiological characteristics, the season of data collection, and reference standards were considered to play a vital role in the final result of the performance of the CareStart™ pLDH/HRP-2 RDT (Woyessa et al., 2013). The present research found low sensitivity for CareStart™ pLDH/HRP-2 and HRP-2 RDT, which agrees with previous study (Woyessa et al., 2013). The low performance of RDT could be due to a low density of malaria parasites and a reduced population of positive participants (Woyessa et al., 2013). The long-term trends of anti-malarial use, as well as the use of counterfeit, less valuable, and unlawful medications, could also be attributed to the progression of the selective pressure on malaria parasites in the blood stream and the consequent low parasitaemia below the kit detection threshold. Furthermore, low performance of the RDT could be a result of the manufacturing process or environmental

conditions (Wongsrichanalai et al., 2007). Maintaining the quality and assurance of malaria RDTs requires keeping perishable medical materials at the appropriate storage temperature and humidity (Chanthap et al., 2010) because abnormal storage conditions could degrade immunochromatographic RDTs (Barbé et al., 2012). Research has demonstrated that some RDTs' performance during their shelf-life is significantly impacted by simulated high temperatures, and prolonged exposure to significant temperatures can cause RDTs to lose acceptable sensitivity or malfunction (Bell et al., 2006). A study has shown that this constraint can be eliminated for malaria case management by using easy, inexpensive, and locally accessible technology (Chanthap et al., 2010). During this study, the low and moderate temperatures in the health facilities seemed to be within a tolerance range for the RDTs, as there was no significant difference between the temperature and the RDTs used in most of the stations. The variability in RDT performance after heat exposure can stem from multiple factors. Although high temperatures are known to denature proteins, but the degree of resistance varies based on protein sequence and structure, which may explain the observed differences in stability (Timr et al., 2020). Additionally, the quality of materials used in the strip itself could contribute to degradation (Ilesanmi et al., 2017). In an analysis done on commercially available RDTs (50) by the world health organization, they found that the stability of 37 was between 2°C – 30°C while the remaining 13 had stability up to 40°C (Albertini et al., 2012). In another study by the same organization, forty-eight malaria RDTs were exposed to heat (45°C) and humidity of 75% for sixty days; the RDTs were used to test malaria. They found that 57.8% had viability under these conditions with *P. falciparum*, while 10% remained viable for *P. vivax* or other malaria parasites (Peeling & Mabey, 2010). In Nigeria and many other African countries, the issue of high temperature is common, as a result, all measures needed to be considered before storing or transporting RDTs from one point to another or within

a health care facility. A study in Brazil which is considered a temperate region, RDTs were stored in a place that is higher than the recommended for fifteen months, the result shows that the sensitivity for *P. falciparum* and *P. vivax* (79.7% and 85.7% respectively) was below the WHO recommended value. Similar results were also reported from Senegal and Ethiopia (Albertini et al., 2012; Gomes et al., 2013). In order to reduce the impact of degradation on RDTs, provision of cold storage facilities in health care facilities and during transportation should be considered at all times. Storage of RDTs in evaporative cooling boxes in Cambodia has resulted in about 97% reduction in the thermal stress and the performance of the RDTs were almost within the desired result; the storage period was also extended from 210 days to close to one year (Chanthap et al., 2010). RDTs stored in temperature, less than 8°C were compared with RDTs stored in an ambient temperature in Afghanistan. The result showed that invalid results were higher in RDTs stored in an ambient temperature compared to the other storage method (Mikhail et al., 2011).

The links between the biomarkers used at the control and test lines of the RDT nitrocellulose strip become weaker in the presence of high humidity (Barbé et al., 2012). Condensation of atmospheric water vapour causes humidity, which is crucial in conditions where high humidity and high temperatures coexist. Meanwhile, condensation will be avoided by using a desiccant to lower the relative humidity inside the device package, as recommended by the WHO. More so, the RDT device should not be utilized if it is saturated; instead, it should be discarded (Cunningham et al., 2020). The significant difference between different levels of relative humidity and the RDTs shows the negative effect of increased relative humidity on the performance of the RDTs used during this study. This agrees with previous studies where high relative humidity reduced the sensitivity, specificity, and accuracy of malaria test kits in Bamako, Mali (Eibach et al., 2013). The effect of

humidity on RDTs cannot be relegated because abnormal humidity could impair the performance of several commercially available RDTs (Crucitti et al., 2011). A study done by Barbé et al. (2012) assessed the effect of desiccant (protect against degradation due to humidity) on RDTs; with package as recommended by WHO and European Community (EC). Their result shows that of the 50 malaria RDT assessed, 22 self-indicating or 8 partial-indicating silica gel contained the toxic cobalt dichloride as humidity indicator. Also, colour change indicating humidity saturation was observed for 8 RDT products of sachets inspected. In addition, they also found that all RDTs with partial-indicating silica gel, sachets with no colour indicating beads were observed, less than half (47%) instruction for use of RDT products with indicating desiccants failed to state that humidity saturation should be checked before using the product, indicating the inability of the RDTs products sampled to meet-up with the international standard required as regard humidity.

The RDTs had a low NPV, making it less reliable for excluding malaria. On the other hand, a greater PPV in this study indicates that patients would receive an accurate malaria diagnosis and avoid needless medication. Likelihood ratio (LR) is a crucial parameter for assessing the precision of a diagnosis and is dependent on the prevalence of the disease condition. It is the proportion of test subjects with a particular disease compared to the expected test result. LR links the likelihood of an illness in a particular patient between the pretest and the posttest (Iwuafor et al., 2018). Positive Likelihood Ratio (PLR) is one of the markers for confirming a diagnosis, but negative Likelihood Ratio (NLR) is a reliable indicator for disconfirming a diagnosis. The higher accuracy of CareStart™ pLDH/HRP-2 RDT over HRP-2 showed better performance of CareStart™ pLDH/HRP-2. However, a higher positive likelihood ratio and negative likelihood ratio of HRP-2



were recorded during this study. Our result is in consonance with similar results in Calabar, South-south Nigeria (Iwuafor et al., 2018).

Inadequate storage and shelf-life management of RDTs can have significant implications. Sensitivity and accuracy may be compromised, leading to false-positive or false-negative results, which impact patient care and malaria prevention efforts (Dejzmach et al., 2021). Inaccurate RDT data can result in misdiagnosis, with false positives causing unnecessary treatments and potential side effects, while false negatives could lead to undertreatment. Improper storage and management can also result in the loss of valuable diagnostic tools, necessitating the disposal of unusable tests and causing direct financial losses for the healthcare system (Engel et al., 2021). This inefficient allocation of resources diverts funds from other critical aspects of malaria control, such as treatment, prevention, or surveillance, to replace unusable RDTs. Additionally, repeated issues with unreliable RDTs due to poor storage can erode healthcare workers' trust in these diagnostic tools, negatively affecting patient care. Poor storage practices can lead to erroneous surveillance data and misdiagnosis, undermining efforts to control and eradicate malaria and exacerbating the disease's spread.

## References

- Abu N, Mohd Bakhori N, & Shueb RH. (2023). Lateral Flow Assay for Hepatitis B Detection: A Review of Current and New Assays. *Micromachines*, 14(6), 1239. <https://doi.org/10.3390/mi14061239>
- Aigbodion I, & Uyi O. (2013). *Temporal distribution of and habitat diversification by some mosquitoes (Diptera: Culicidae) species in Benin City, Nigeria*. 10(1), 13–23.

- Ajakaye OG, & Ibukunoluwa MR. (2020). Prevalence and risk of malaria, anemia and malnutrition among children in IDPs camp in Edo State, Nigeria. *Parasite Epidemiology and Control*, 8, e00127. <https://doi.org/10.1016/j.parepi.2019.e00127>
- Albertini A, Lee E, Coulibaly SO, Sleshi M, Faye B, Mationg ML, Ouedraogo K., Tsadik AG, Feleke SM, Diallo I, Gaye O, Luchavez J, Bennett J, & Bell D. (2012). Malaria rapid diagnostic test transport and storage conditions in Burkina Faso, Senegal, Ethiopia and the Philippines. *Malaria Journal*, 11(1), 406. <https://doi.org/10.1186/1475-2875-11-406>
- Barbé B, Gillet P, Beelaert G, Franssen K, & Jacobs J. (2012). Assessment of desiccants and their instructions for use in rapid diagnostic tests. *Malaria Journal*, 11. <https://doi.org/10.1186/1475-2875-11-326>
- Barber BE, William T, Grigg MJ, Menon J, Auburn S, Marfurt J, Anstey NM. & Yeo TW. (2013). A Prospective Comparative Study of Knowlesi, Falciparum, and Vivax Malaria in Sabah, Malaysia: High Proportion With Severe Disease From Plasmodium Knowlesi and Plasmodium Vivax But No Mortality With Early Referral and Artesunate Therapy. *Clinical Infectious Diseases*, 56(3), 383–397. <https://doi.org/10.1093/cid/cis902>
- Bell D, Wongsrichanalai C, & Barnwell JW. (2006). Ensuring quality and access for malaria diagnosis: How can it be achieved? *Nature Reviews Microbiology*, 4(9), 682–695. <https://doi.org/10.1038/nrmicro1474>
- Bouyou-Akotet MK, Mawili Mboumba DP, Kendjo E, Mbadinga F, Obiang-Bekale N, Mouidi P, & Kombila M. (2013). Anaemia and severe malarial anaemia burden in febrile Gabonese children: A nine-year health facility based survey. *The Journal of Infection in Developing Countries*, 7(12), 983–989. <https://doi.org/10.3855/jidc.3347>

- Brunner NC, Omoluabi E, Awor P, Okitawutshu J, Tshefu Kitoto A, Signorell A, Akano B, Ayodeji, K, Okon C, Yusuf O, Athieno P, Kimera J, Tumukunde G, Angiro I, Kalenga JC, Delvento G, Lee TT, Lambiris MJ, Ross A, Hetzel MW. (2022). Prereferral rectal artesunate and referral completion among children with suspected severe malaria in the Democratic Republic of the Congo, Nigeria and Uganda. *BMJ Global Health*, 7(5), e008346. <https://doi.org/10.1136/bmjgh-2021-008346>
- Chanthap L, Ariey F, Socheat D, Tsuyuoka R, & Bell D. (2010). Low-technology cooling box for storage of malaria RDTs and other medical supplies in remote areas. *Malaria Journal*, 9(1). <https://doi.org/10.1186/1475-2875-9-31>
- Chiodini PL, Bowers K, Jorgensen P, Barnwell JW, Grady KK, Luchavez J, Moody AH, Cenizal A, & Bell D. (2007). The heat stability of Plasmodium lactate dehydrogenase-based and histidine-rich protein 2-based malaria rapid diagnostic tests. *Transactions of the Royal Society of Tropical Medicine and Hygiene*, 101(4), 331–337. <https://doi.org/10.1016/j.trstmh.2006.09.007>
- Crucitti T, Taylor D, Beelaert G, Fransen K, & Van Damme L. (2011). Performance of a Rapid and Simple HIV Testing Algorithm in a Multicenter Phase III Microbicide Clinical Trial. *Clinical and Vaccine Immunology*, 18(9), 1480–1485. <https://doi.org/10.1128/CVI.05069-11>
- Cunningham JA, Thomson RM, Murphy SC, De La Paz Ade M, Ding XC, Incardona S, Legrand E, Lucchi NW, Menard D, Nsobya SL, Saez AC, Chiodini PL, & Shrivastava J. (2020). WHO malaria nucleic acid amplification test external quality assessment scheme: Results of distribution programmes one to three. *Malaria Journal*, 19(1), 129. <https://doi.org/10.1186/s12936-020-03200-0>

- Dejzmach Z, Alemu G, Yimer M, Tegegne B, & Getaneh A. (2021). Prevalence of Malaria and Associated Knowledge, Attitude, and Practice among Suspected Patients in Bahir Dar Zuria District, Northwest Ethiopia. *BioMed Research International*, 2021, 1–11. <https://doi.org/10.1155/2021/3741413>
- Eibach D, Traore B, Bouchrik M, Coulibaly B, Coulibaly N, Siby F, Bonnot G, Bienvenu A, & Picot S. (2013). Evaluation of the malaria rapid diagnostic test VIKIA malaria Ag Pf/Pan™ in endemic and non-endemic settings. *Malaria Journal*, 12(1), 188. <https://doi.org/10.1186/1475-2875-12-188>
- Engel N, Ghergu C, Matin MA, Kibria MG, Thriemer K, Price RN, Ding XC, Howes RE, Ley B, Incardona S, & Alam MS. (2021). Implementing radical cure diagnostics for malaria: User perspectives on G6PD testing in Bangladesh. *Malaria Journal*, 20(1), 217. <https://doi.org/10.1186/s12936-021-03743-w>
- Gomes LT, Tada MS, Katsuragawa TH, Povoia MM, Viana GM, Alecrim MDGC, De Santana-Filho FS, Arcanjo ARL, Couto AARA, Calvosa VSP, Nery AF, & Fontes CJF. (2013). Low sensitivity of malaria rapid diagnostic tests stored at room temperature in the Brazilian Amazon Region. *The Journal of Infection in Developing Countries*, 7(03), 243–252. <https://doi.org/10.3855/jidc.2564>
- Ilesanmi RI, Olalubi OA, Adetunde OT, Ilesanmi AO, Effedua H, & Amoo AO. (2017). Comparative assessment of malaria rapid diagnostic tests (RDT) in Ibadan, Nigeria. *MalariaWorld Journal*, 8, 17.
- Iwuafor A, Ita O, Ogban G, Udoh U, & Amajor C. (2018). Evaluation of diagnostic accuracy of rapid diagnostic test for malaria diagnosis among febrile children in Calabar, Nigeria. *Nigerian Medical Journal*, 59(6), 64. [https://doi.org/10.4103/nmj.NMJ\\_165\\_18](https://doi.org/10.4103/nmj.NMJ_165_18)

- Martiáñez-Vendrell X, Skjefte M, Sikka R, & Gupta H. (2022). Factors Affecting the Performance of HRP2-Based Malaria Rapid Diagnostic Tests. *Tropical Medicine and Infectious Disease*, 7(10), Article 10. <https://doi.org/10.3390/tropicalmed7100265>
- Mikhail AF, Leslie TJ, Mayan MI, Zekria R, Mohammad N, Hasanzai MA, Safi N, Whitty CJ, & Rowland M. (2011). Field trial of three different Plasmodium vivax- detecting rapid diagnostic tests with and without evaporative cool box storage in Afghanistan. *Malaria Journal*, 10(1), 169. <https://doi.org/10.1186/1475-2875-10-169>
- Morakinyo OM, Balogun FM, & Fagbamigbe AF. (2018). Housing type and risk of malaria among under-five children in Nigeria: Evidence from the malaria indicator survey. *Malaria Journal*, 17(1), 311. <https://doi.org/10.1186/s12936-018-2463-6>
- Oboh MA, Oriero EC, Ndiaye T, Badiane AS, Ndiaye D, & Amambua-Ngwa A. (2021). Comparative analysis of four malaria diagnostic tools and implications for malaria treatment in southwestern Nigeria. *International Journal of Infectious Diseases*, 108, 377–381. <https://doi.org/10.1016/j.ijid.2021.05.049>
- Oladosu O, Adedokun V, Adeniyi A, & Oyibo W. (2021). *Performance Evaluation of Malaria HRP-2 Rapid Diagnostic Test among Febrile Patients with Malaria in Iwo, Osun State, Nigeria*. 4, 046.
- Peeling RW, & Mabey D. (2010). Point-of-care tests for diagnosing infections in the developing world. *Clinical Microbiology and Infection*, 16(8), 1062–1069. <https://doi.org/10.1111/j.1469-0691.2010.03279.x>
- Persing Tenover, Hayden, Ieven, Miller, Nolte, Tang, & Van Belkum (Eds.). (2016). Rapid Point-of-Care Diagnosis of Malaria and Dengue Infection. In *Molecular Microbiology* (pp. 589–609). American Society of Microbiology. <https://doi.org/10.1128/9781555819071.ch42>

- Temiloluwa A, Williams OT, Azeez GI, & Huldah O. (2023). Assessment of the Knowledge, Attitude, Practices and Malaria Prevalence among Undergraduates. *International Journal of Tropical Diseases*, 6(1). <https://doi.org/10.23937/2643-461X/1710069>
- Timr S, Madern D, & Sterpone F. (2020). Protein thermal stability. In *Progress in Molecular Biology and Translational Science* (Vol. 170, pp. 239–272). Elsevier. <https://doi.org/10.1016/bs.pmbts.2019.12.007>
- Uba CC, Ikegbunam MN, Anagor IS, Eleanya LC, Ezeumeh EN, Ezekwueche SN, Okechukwu E. C, & Esimone, CO. (2021). Comparative Performance of Different Malaria Diagnostic Tools among Pregnant Cohorts in Onitsha Southeast Nigeria. *Advances in Infectious Diseases*, 11(04), 384–394. <https://doi.org/10.4236/aid.2021.114035>
- Venkatesan P. (2024). The 2023 WHO World malaria report. *The Lancet Microbe*, 5(3), e214. [https://doi.org/10.1016/S2666-5247\(24\)00016-8](https://doi.org/10.1016/S2666-5247(24)00016-8)
- Williams GS, Mweya C, Stewart L, Mtove G, Reyburn H, Cook J, Corran PH, Riley EM, & Drakeley CJ. (2009). Immunophoretic rapid diagnostic tests as a source of immunoglobulins for estimating malaria sero-prevalence and transmission intensity. *Malaria Journal*, 8(1), 168. <https://doi.org/10.1186/1475-2875-8-168>
- Wongsrichanalai C, Barcus J, Muth S, Sutamihardja A, & Wernsdorfer W. (2007). *A review of malaria diagnostic tools: Microscopy and rapid diagnostic test (RDT). Defining and Defeating the Intolerable Burden of Malaria III: Progress and Perspectives*. 77(6), 1–28.
- Woyessa A, Deressa W, Ali A, & Lindtjörn B. (2013). Evaluation of CareStart™ malaria Pf/Pv combo test for Plasmodium falciparum and Plasmodium vivax malaria diagnosis in Butajira area, south-central Ethiopia. *Malaria Journal*, 12(1). <https://doi.org/10.1186/1475-2875-12-218>